

Fig. 1

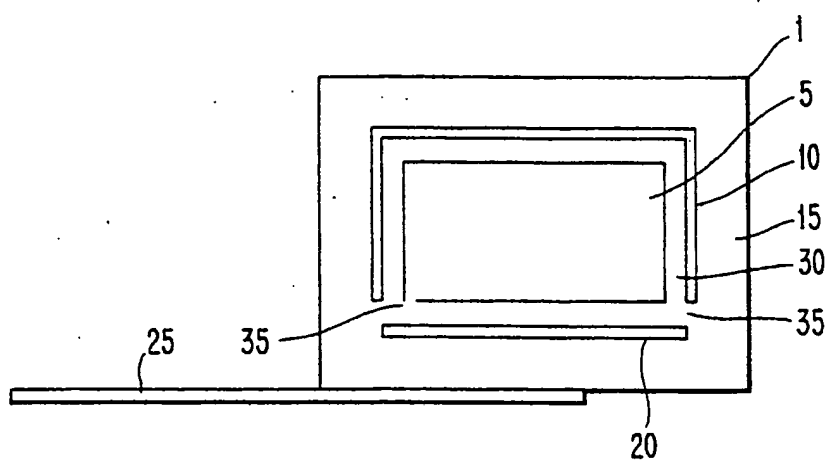
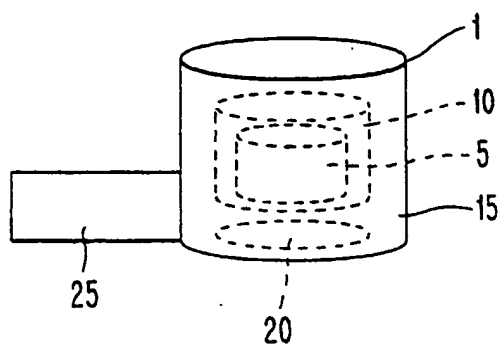


Fig. 2

Figure 3

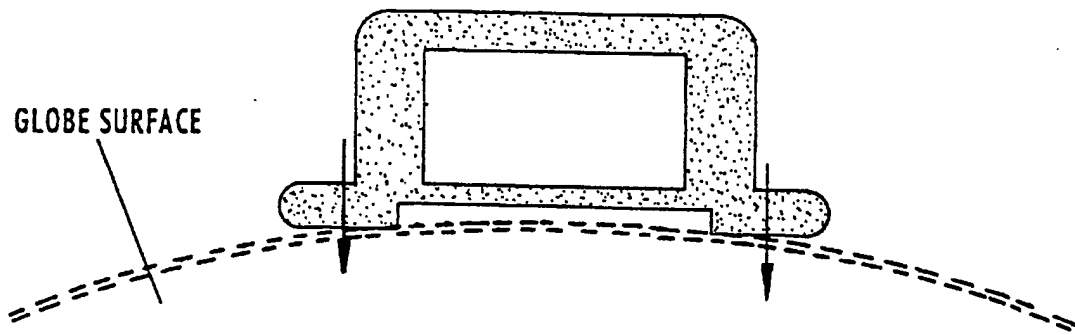
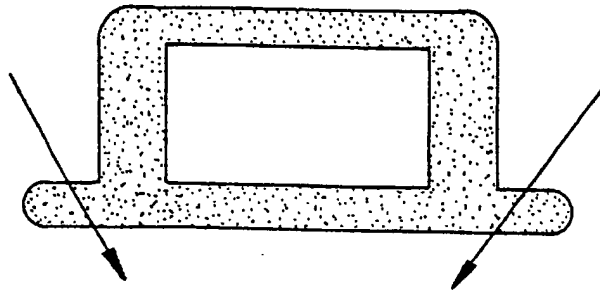
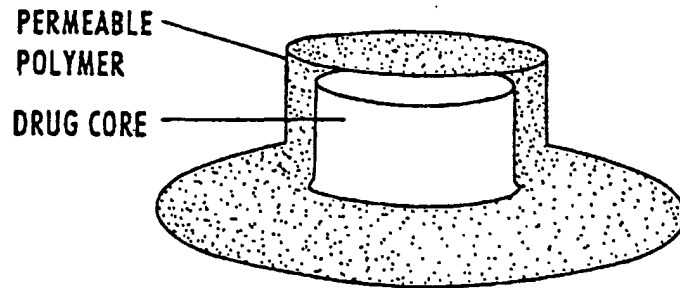


Figure 4

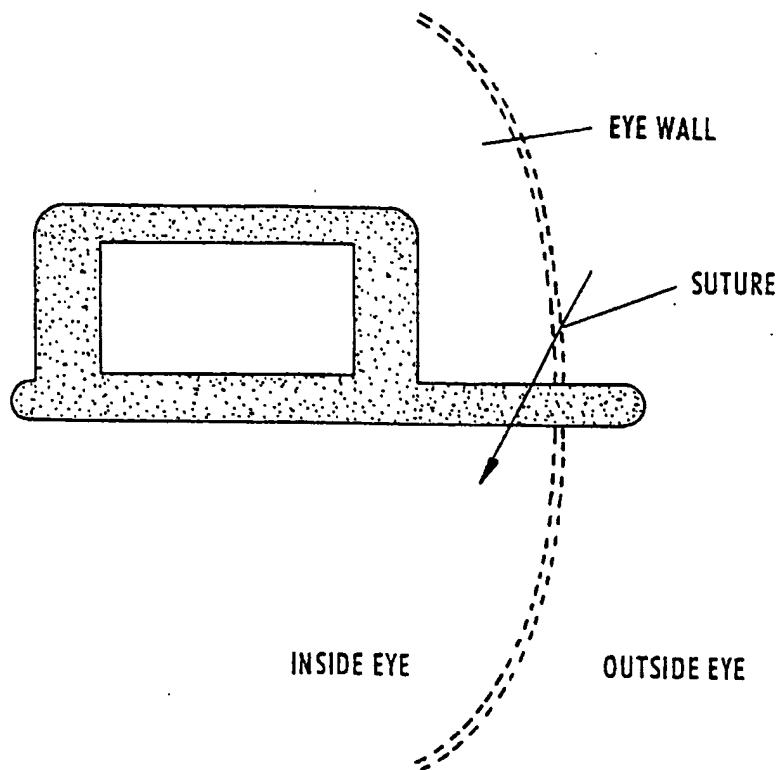
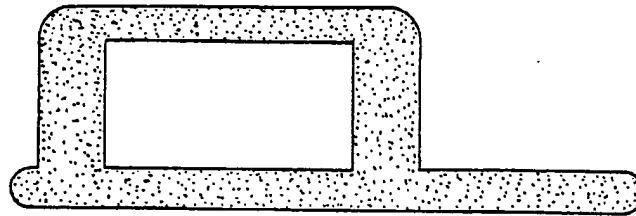
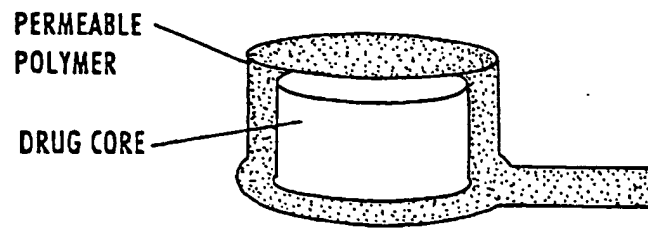


Figure 5

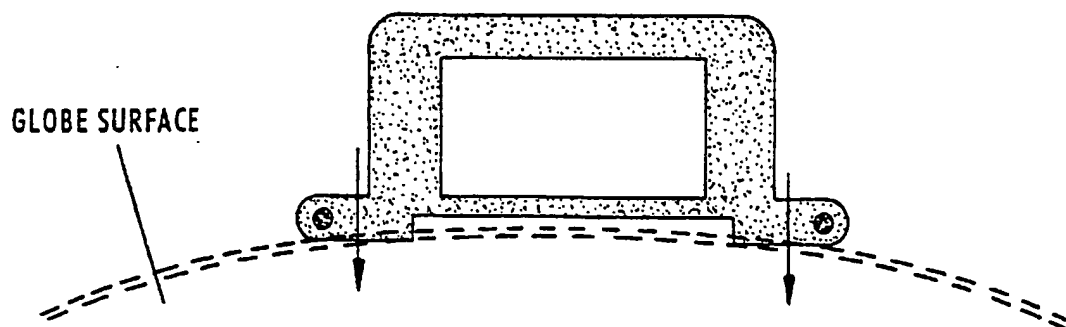
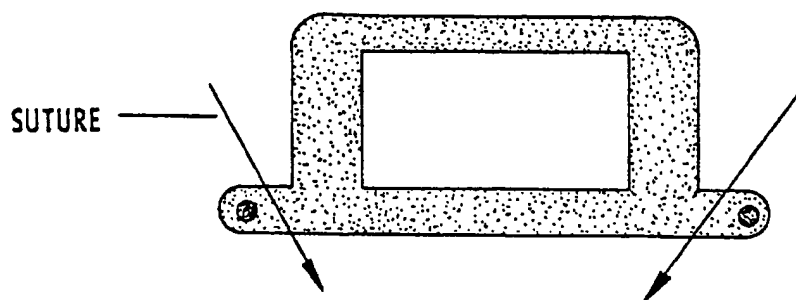
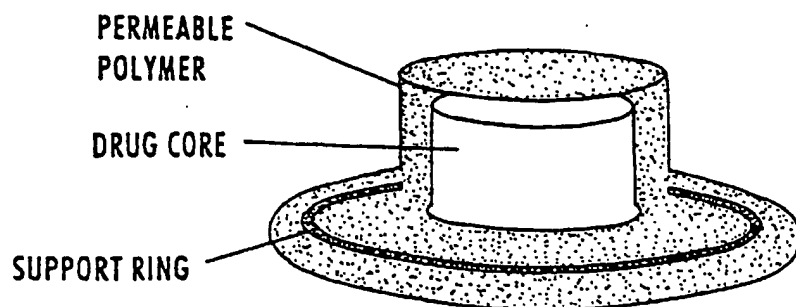


Figure 6

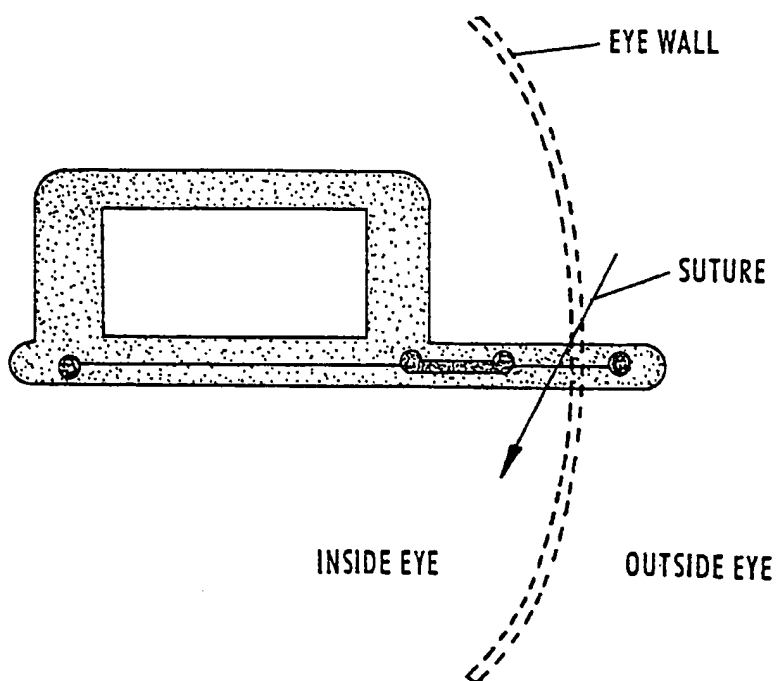
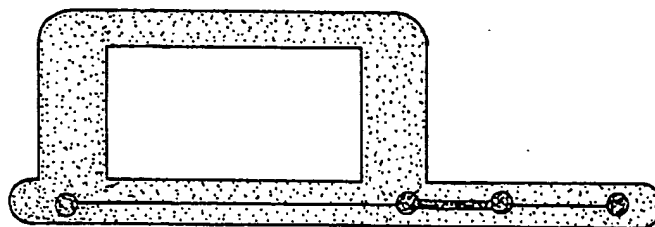
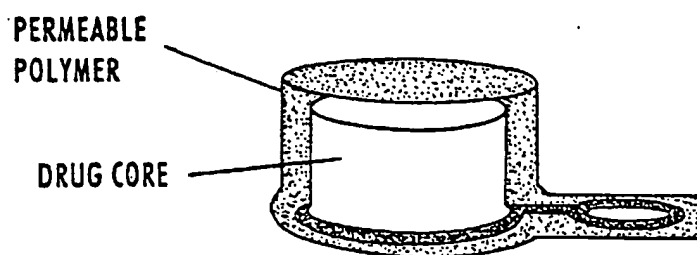


Figure 7

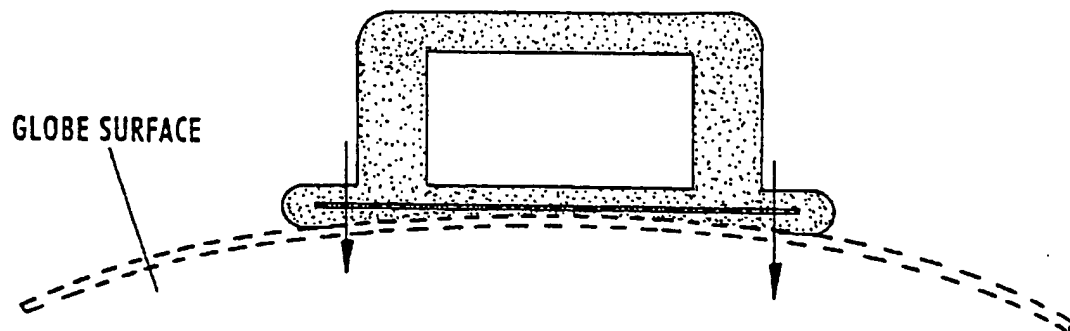
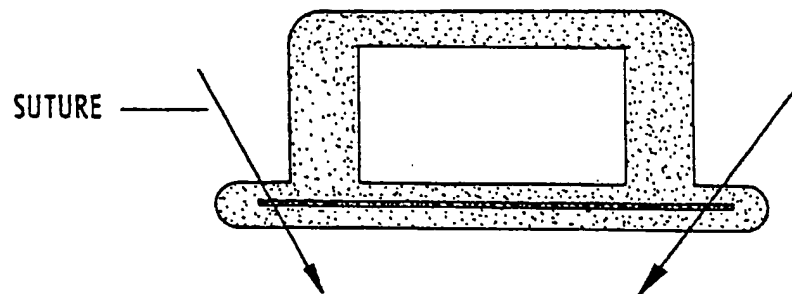
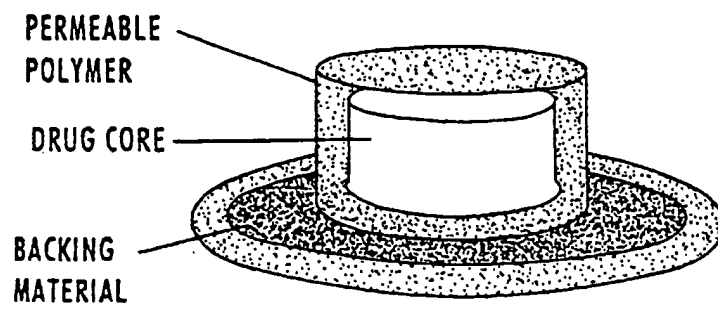
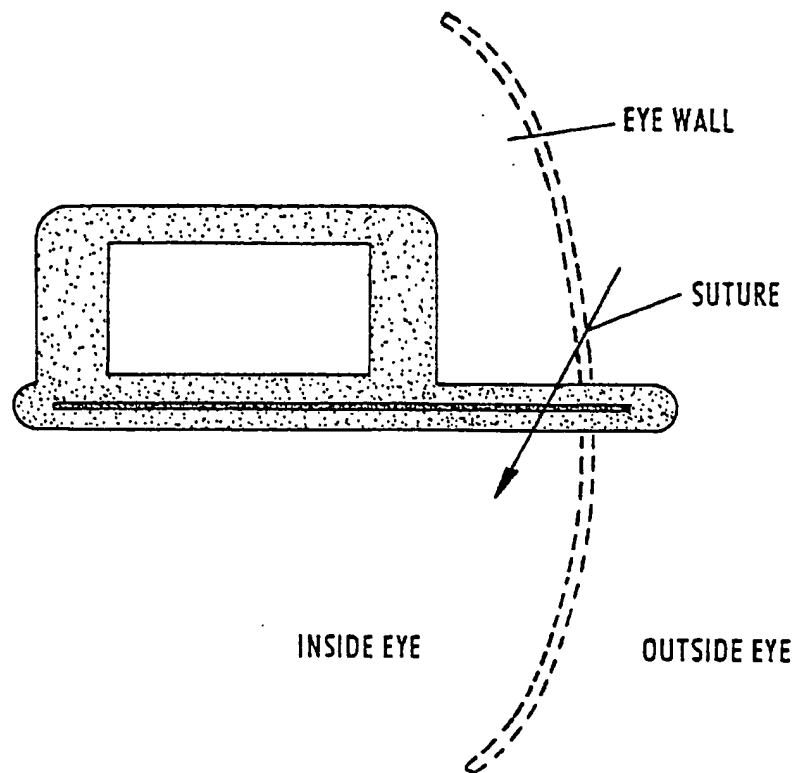
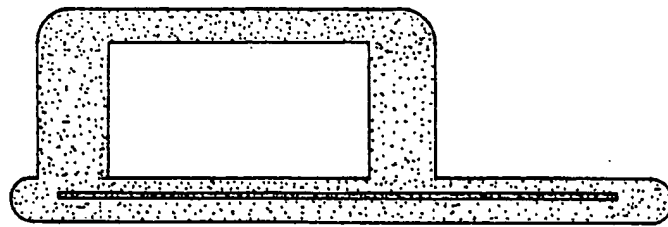
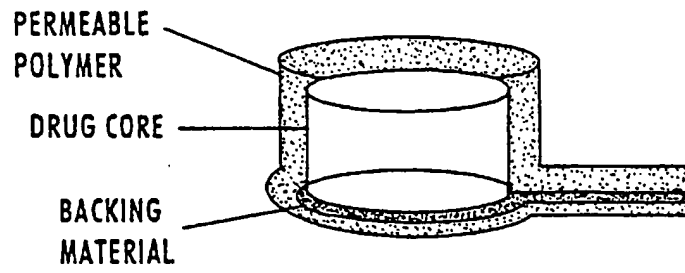


Figure 8



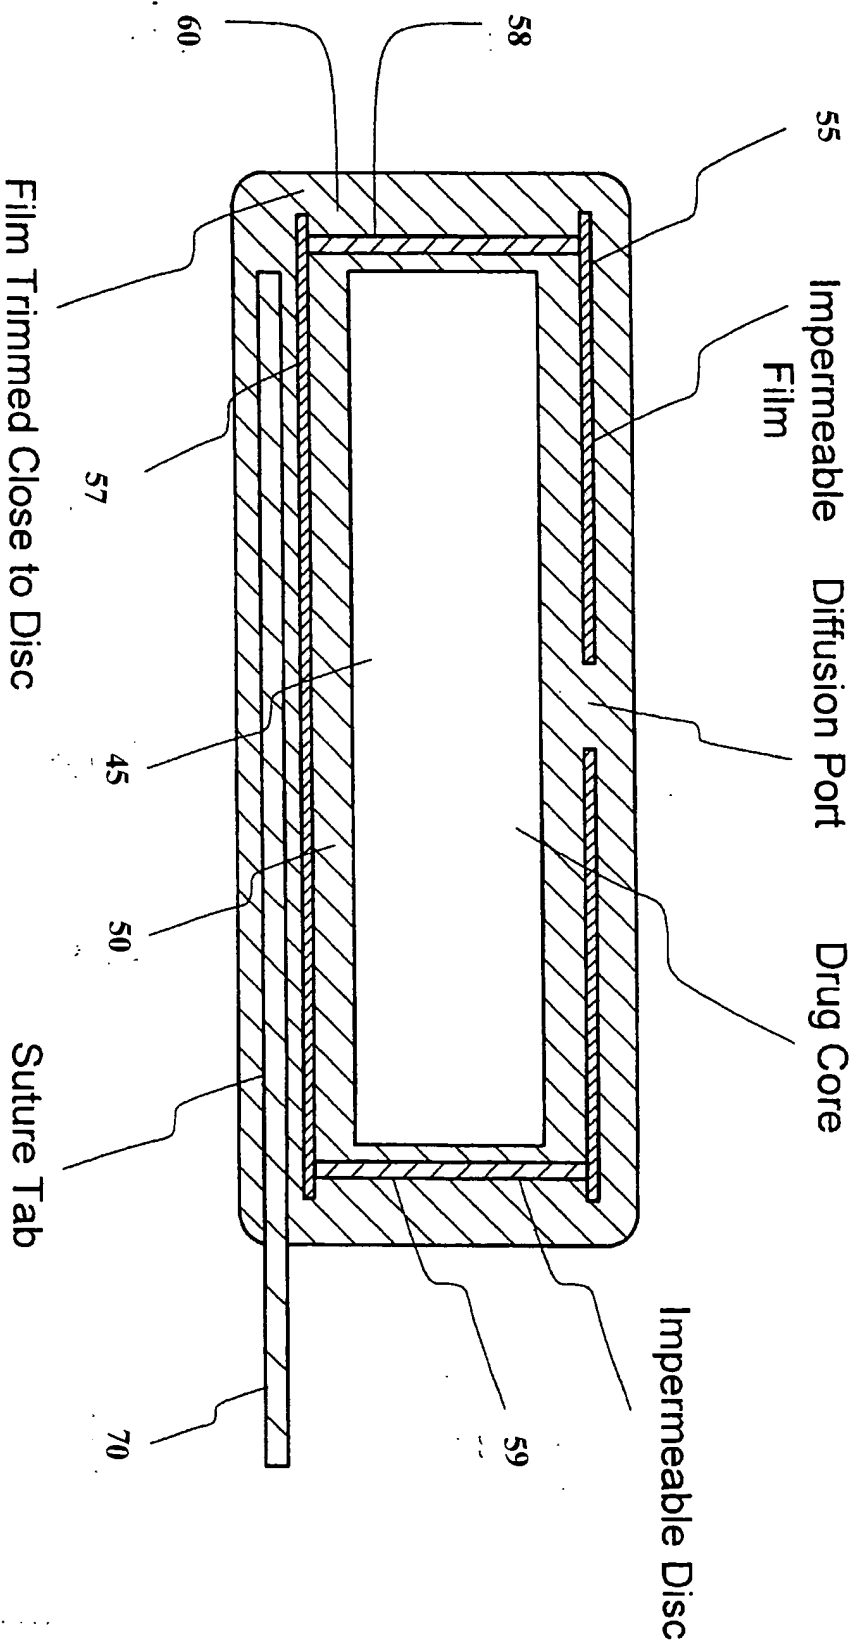


FIG. 9

Advantages of End Discs

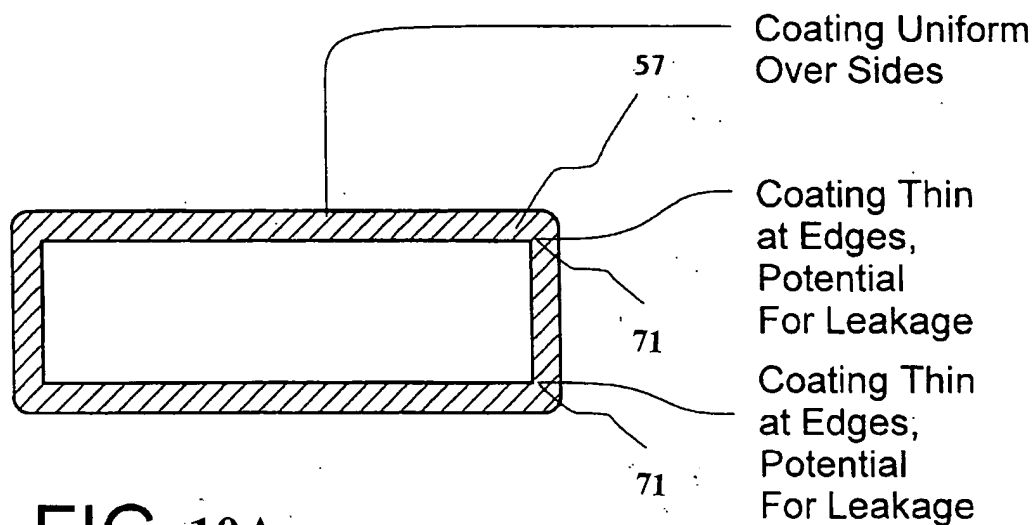


FIG. 10A

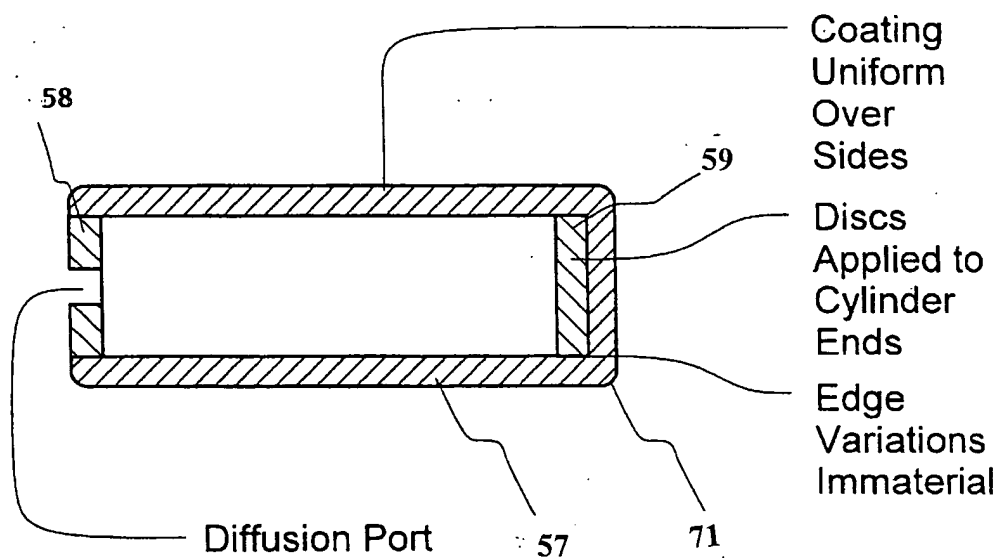


FIG. 10B

For clarity only the second (impermeable)
coating film is shown

2mg Fluocinolone acetonide implants
in buffer (ph 7.4) release profile

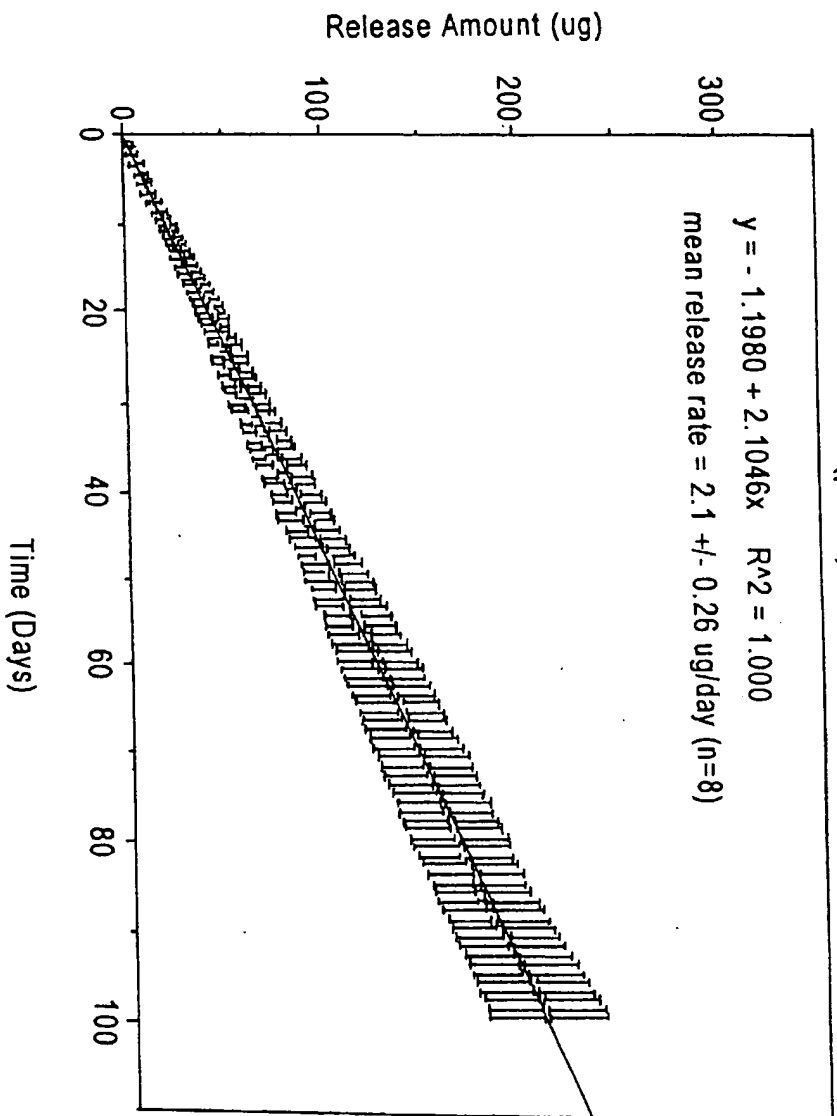


FIG. 11

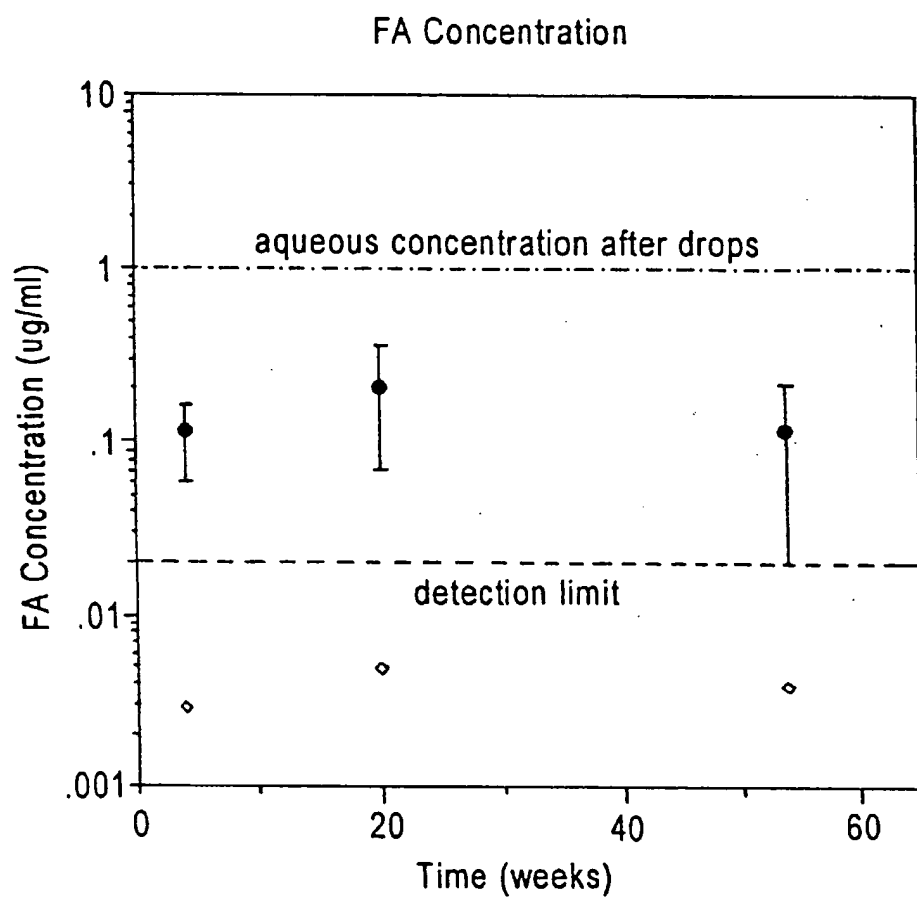


FIG. 12